

(19)



Europäisches Patentamt

European Patent Office

Office européen des brevets



(11)

EP 1 243 283 A2

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:

25.09.2002 Bulletin 2002/39

(51) Int Cl.7: A61M 25/00, A61M 25/01

(21) Application number: 02251981.3

(22) Date of filing: 20.03.2002

(84) Designated Contracting States:

AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR

Designated Extension States:

AL LT LV MK RO SI

(30) Priority: 21.03.2001 JP 2001081416

10.08.2001 JP 2001243937

(71) Applicant: ASAHI INTECC CO., LTD.

Nagoya-shi, Aichi-ken (JP)

(72) Inventors:

- Miyata, Naohiko, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Kato, Tomihisa, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Miyata, Kenji, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)

- Osawa, Toshiya c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Matsuo, Kazumi c/c ASAHI INTECC CO LTD., Nagoya-shi, Aichi-ken (JP)
- Kusuda, Ryuji c/o ASAHI INTECC CO LTD., Nagoya-shi, Aichi-ken (JP)
- Nakagoshi, Yoshinobu c/oASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Kato, Tadakazu c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)


(74) Representative: Senior, Alan Murray

J.A. KEMP & CO.,
14 South Square,
Gray's Inn
London WC1R 5JJ (GB)

(54) A wire-stranded hollow tube, a medical tube body and a medical guide wire

(57) In a wire-stranded hollow tube 1, a plurality of metallic wires (8) preformed with a predetermined forming rate are twisted along a circular line into a coreless hollow configuration. When twisting the metallic wires (8), the neighboring metallic elements (1a, 1a) are subjected to compression with no gap appeared between the neighboring metallic elements (1a, 1a). This increases a contact pressure between the neighboring metallic elements (1a, 1a) to attain a good tightness with a good circularity and diametrical uniformity, and thereby preventing the wire-stranded hollow tube 1 from inadvertently collapsing. A tightness is strengthened between the neighboring metallic elements (1a, 1a) when the metallic elements (1a, 1a) of different helical pitch are used. By applying the wire-stranded hollow tube 1 to a medical guide wire, a quick torque response and a good torque transmissibility are ensured which leads to a good manipulatability with a favorable follow-on capability.

Fig. 2

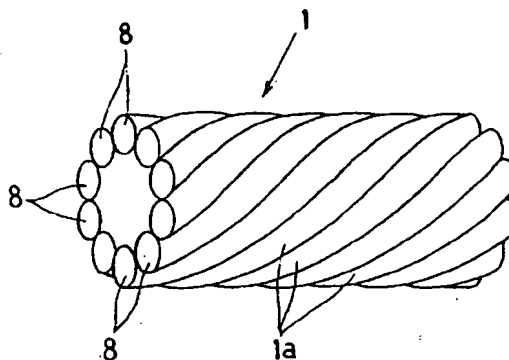

EP 1 243 283 A2

Description

[0001] The invention relates to a wire-stranded hollow tube in which a plurality of metallic wires are twisted along a circular line to be shaped into a coreless hollow configuration, and particularly concerns to a medical tube body and a medical guide wire into which the wire-stranded hollow tube is incorporated.

[0002] As a general medical tube body, a synthetic resin tube and a flexible tube (T) has been introduced in which a helical spring (S) is embedded in a synthetic resin (P) as shown in Fig. 34. The helical spring (S) is single wound or multiple wound by a spring forming machine. To take a five-turn wound helical spring (U) as an example in Fig. 35, a gap (G) is likely to appear at every five-turn wound end (N). The gap (G) develops remarkably in particular when an initial winding tension is not enough upon forming the helical spring (U).

[0003] This not only imparts the helical spring (U) with a convexo-concave outer appearance but result in a loss of torque under the presence of the gap (G) when transmitting the torque through the helical spring (U). An accumulated loss of the torque exceedingly reduces the torque transmissibility. On the other hand, the helical spring (U) increases its rigidity when the initial winding tension is strengthened too much upon forming the helical spring (U). Under the increased rigidity, the frictional resistance increases between the helical spring (U) and an inner wall of a wound and small blood vessel every time when advancing the helical spring (U) to pass through wound portions of the wound and small blood vessel. The increased frictional resistance deteriorates a manipulatability when the helical spring (U) is applied to a medical guide wire.

[0004] A Laid-open Japanese Patent Application No. 11-25758 (prior reference) discloses a wire-stranded hollow body in which wire elements are twisted along a circle line to overcome the drawbacks which a multiple coaxial cable wire usually has, so as to attain a lightweight structure with a smooth surface and a good circularity. The wire-stranded hollow body disclosed by the prior reference, however, is applied practically to an electric cable wire and has no substantial suggestion about an improved tightness between the wire elements to ensure a quick torque response and a good torque transmissibility.

[0005] Therefore, the present invention has been made with the above disadvantages in mind, it is a main object of the invention to provide a medical tube body and a medical guide wire which has a wire-stranded hollow tube formed by a plurality of metallic wires twisted along a circular line into a coreless hollow configuration with no gap appeared between the neighboring metallic wires by increasing a contact pressure therebetween to attain a good tightness between the neighboring metallic wires with a good circularity and a good diametrical uniformity to ensure a quick torque response and good torque transmissibility with the least play, thereby lead-

ing to a good manipulatability with a favorable follow-on capability.

[0006] According to the present invention, there is provided a wire-stranded hollow tube in which a plurality of metallic wires are twisted along a circular line to be a coreless hollow configuration with the metallic wires preformed by a predetermined forming rate (forming strain). This provides a uniform contact pressure between the neighboring metallic wires with no gap appeared therebetween. The contact pressure between the neighboring metallic wires can be strengthened by increasing a helical pitch (e.g., 7 ~ 8 times the line diameter of the metallic wires) of the metallic wires.

[0007] With the increased contact pressure between the neighboring metallic wires, a good tightness between the neighboring metallic wires is ensured to tightly unite the metallic wires together with a good circularity and a good diametrical uniformity. Providing a postforming treatment with the wire-stranded hollow tube unites the metallic wires all the more tightly together to prevent the wire-stranded hollow tube from inadvertently collapsing. With the forming rate in the range of 90 ~ 98% when preforming the metallic wires, the good circularity and the good diametrical uniformity are strengthened.

[0008] According to other aspect of the invention, the metallic wires are formed from different materials. The circularity and the diametrical uniformity are all the more improved.

[0009] According to other aspect of the invention, the wire-stranded hollow tube is incorporated into a medical tube body and a medical guide wire. At the time of manipulating the medical tube body and medical guide wire, a good manipulatability can be ensured with a quick torque response and a good torque transmissibility achieved with the least play permitted.

[0010] By using the wire-stranded hollow tube, the good manipulatability can be ensured with the quick torque response and the good torque transmissibility secured with the least play at the time of manipulating the medical guide wire. A helical convexo-concave undulation appeared on an outer surface of the wire-stranded hollow tube enables a manipulator to a firm grip with no finger slip so as to readily introduce the medical guide wire to reach a target area. According to other aspect of the invention, a single elastic elongation core is placed within a hollow portion of the wire-stranded hollow tube. This provides the medical guide wire with an improved pushability when inserting the medical guide wire deep into human body.

[0011] A synthetic resin layer is coated with an outer extension of the elongation core. The synthetic resin layer serves as a protection for the elongation core, and at the same time, providing the medical guide wire with a smoothness and a thrombus-repellent property. Adding an X-ray impervious agent (radiopaque agent) to the synthetic resin layer enables the manipulator to an X-ray photography. A hydrophilic resin film coated with the synthetic resin layer increases the smoothness and

the thrombus-repellent property.

[0012] According to other aspect of the invention, a metallic helical spring is wound around a front end of the outer extension. The metallic helical spring contains a radiation-impervious agent. This enables the manipulator to confirm a leading end of the medical guide wire with a good flexibility maintained in the medical guide wire.

[0013] With the metallic helical spring wound around the outer extension by its entire axial length, the flexibility increases compared to the case in which the outer extension is coated with the synthetic resin layer. This flexibility makes it possible to flexibly follow the outer extension along a wound and small blood vessel, and whereby smoothly introducing the medical guide wire deep into the wound and small blood vessel.

[0014] According to other aspect of the invention, a synthetic resin layer is coated with an outer surface of the wire-stranded tube, and a hydrophilic resin film is provided on the synthetic resin layer. This provides the medical guide wire with an increased smoothness and thrombus-repellent property.

[0015] According to other aspect of the invention, the wire-stranded hollow tube is formed of different metallic wires. One is a Ni-Ti alloy wire and the other is a stainless steel wire (material stipulated by SUS) to cite an example. When these two different wires are subjected to diameter-reduction by means of a swaging or die drawing work, the hard Ni-Ti alloy wire tightly engages against the stainless steel wire to plastically deform the stainless steel wire. This increases a contact area between the Ni-Ti alloy wire and the stainless steel wire to more tightly unite these metallic wires together so as to strengthen the torque transmissibility, compared to the case in which the metallic wires are of the same material and of the identical hardness.

[0016] According to other aspect of the invention, the wire-stranded hollow tubes are concentrically arranged to form a multilayered configuration. The multilayered structure provides the medical guide wire with a flexibility, a durability and a stable manipulability in the winding direction.

[0017] According to other aspect of the invention, a pressure sensor is incorporated into the medical guide wire to measure a blood pressure upon inserting the medical guide wire into the blood vessel. When the medical guide wire is inserted into the wound and small blood vessel, the wire-stranded hollow tube keeps its cross section substantially circular at the wound portions without deforming into a flat configuration. Keeping the circular cross section permits blood streams smoothly without disturbing them, thus enabling the manipulator to a precise blood pressure measurement and monitoring for an extended period of time with the least variation.

[0018] A preferred form of the present invention is illustrated in the accompanying drawings in which:

Figs. 1, 1a, 1b and 1c are explanatory views comparatively showing how working transmutation layers are induced when a coil forming machine and a rope stranding machine are used;

Fig. 2 is a perspective view of a wire-stranded hollow tube according to a first embodiment of the invention;

Fig. 3 is a schematic view showing how the wire-stranded hollow tube is formed;

Fig. 4 is a graphical representation showing a rotational angle when each piece starts to rotate;

Fig. 5 is a graphical representation showing a rotational torque when each piece starts to rotate;

Fig. 6 is a graphical representation showing a linear characteristics when each piece starts to rotate in a normal direction;

Fig. 7 is a graphical representation showing a linear characteristics when each piece starts to rotate in a reverse direction;

Fig. 8 is a graphical representation showing a load efficiency represented by a total bending angle when load is applied;

Fig. 9 is a perspective view of the medical guide wire;

Fig. 10 is a perspective view of the medical guide wire when a thermoplastic synthetic resin layer and a hydrophilic resin film is coated with the medical guide wire;

Fig. 11 is a plan view of a balloon catheter;

Fig. 12 is an enlarged cross section taken along the line R-R of Fig. 11;

Fig. 13 is a perspective view of the wire-stranded hollow tube subjected to a die drawing work;

Fig. 14 is a perspective view of a modified wire-stranded hollow tube;

Fig. 15 is a schematic view comparatively showing the wire-stranded hollow tube subjected to a diameter reduction;

Fig. 16 is a perspective view of a medical guide wire in which the wire-stranded hollow tube is applied to the medical guide wire according to a second embodiment of the invention;

Fig. 17 is a perspective view of a medical guide wire in which the wire-stranded hollow tube is applied to the medical guide wire according to a third embodiment of the invention;

Fig. 18 is an enlarged longitudinal cross sectional view showing a circled portion E of Fig. 17;

Fig. 19 is an enlarged longitudinal cross sectional view showing a circled portion F of Fig. 17;

Fig. 20 is an enlarged longitudinal cross sectional view showing a circled portion G of Fig. 17;

Fig. 21 is an enlarged latitudinal cross sectional view taken along the line A-A of Fig. 17;

Fig. 22 is a perspective view of a medical guide wire in which the wire-stranded hollow tube is applied to the medical guide wire according to a fourth embodiment of the invention;

Fig. 23 is an enlarged longitudinal cross sectional view taken along the line Y-Y of Fig. 22;

Fig. 24 is an enlarged longitudinal cross sectional view taken along the line X-X of Fig. 22;

Fig. 25 is a perspective view of a medical guide wire according to a fifth embodiment of the invention;

Fig. 26 is a perspective view of a medical guide wire according to a sixth embodiment of the invention;

Fig. 27 is a perspective view of a medical guide wire according to a seventh embodiment of the invention;

Fig. 28 is a schematic view showing how a general medical tube works when inserted into a wound and small blood vessel;

Fig. 29 is a schematic view showing how the general tube disturbs blood streams;

Fig. 30 is a schematic view of the medical guide wire which is advanced into the wound and small blood vessel 1;

Fig. 31 is a schematic view of a single wound helical spring bent along the wound and small blood vessel;

Fig. 32 is a schematic view of the wire-stranded hollow tube bent along the wound and small blood vessel;

Fig. 33 is a schematic view showing how an axial length of the single wound helical spring is stretched;

Fig. 34 is a perspective view of a prior medical tube body formed by a helical spring; and

Fig. 35 is a plan view of the prior medical tube body formed by a helical spring.

[0019] According to a first embodiment of the invention, a wire-stranded hollow tube 1 (Fig. 2) is in a strand structure in which a plurality of metallic wires 8 are placed along a circular line and twisted with the use of a rope twisting machine.

[0020] Upon deforming a metallic wire 2 with the use of a coil forming machine as shown in Figs. 1 and 1a, an inner side of the metallic wire 2 tightly engages against an elevated pin 3, and an outer side of the metallic wire 2 tightly engages against a guide plate 4. This likely produces a working transmutation layer (H) on both sides 2a, 2b of the metallic wire 2.

[0021] Upon deforming a metallic wire 8 with the use of the rope twisting machine as shown in Figs. 1b and 1c, the metallic wire 8 is twisted while being pulled upon weaving through three guide pins 5, 6 and 7 at the time when preforming the metallic wire 8. This provides the working transmutation layer (H) on an entire surface of the metallic wire 8. Upon preforming the metallic wire 8, a forming rate (forming strain) falls in the range of 90 ~ 98 % (preferably 90 ~ 95 %). This provides the metallic wire 8 with an increased flexibility, an improved wear-resistance while removing a residual stress due to the metallic wire 8 being twisted. Releasing the residual stress prevents a spring-back and jumping-out phenom-

ena when severing the metallic wire 8 at a predetermined length.

[0022] The metallic wires 8 are twisted along the circular line to form the wire-stranded hollow tube 1 with the use of the rope twisting machine. Neighboring line elements 1a,

[0023] 1a of the metallic wires 8 engage tightly each other without generating any gap therebetween because the neighboring line elements 1a, 1a are subjected to compression force when twisted. A helical pitch (corresponding to a screw lead) is determined to be 7 ~ 8 times larger than the line diameter of the metallic wire 8 (e.g., $0.43 \times (7 \sim 8) = 3.01 \sim 3.44$ mm).

[0024] Upon postforming a rope structure which passes through a voice tool 9 as shown in Fig. 2, the rope structure is rolled between rollers 10, 10 to form the wire-stranded hollow tube 1 which ensures a good circularity and a good diametrical uniformity.

[0025] Namely, the rope structure thus stretched is severed at an appropriate length, and the core wires are withdrawn from the rope structure in which the metallic wires 8 were wound around the core wires. As the core wires, a bundle of soft line wires (e.g., mild steel) can be used so that the core wires are easily withdrawn. Alternatively, any line member can be used, an outer diameter of which is smaller than an inner diameter of the wire-stranded hollow tube 1.

[0026] The neighboring line elements 1a, 1a are tightly compressed to increase a contact pressure therebetween to unite the metallic wires 8 together, thus preventing the wire-stranded hollow tube 1 from inadvertently collapsing. With the neighboring line elements 1a, 1a tightly engaged each other, a good torque transmissibility can be achieved with a good wetting relationship secured between the neighboring line elements 1a, 1a.

[0027] It is to be noted that a tensile, compression or winding type preforming method may be used, otherwise a preforming method can also be used in which a difference of speed is converted to a tensile force.

[0028] From a view point of performance, the wire-stranded hollow tube 1 is compared to other counterpart pieces.

[0029] The following relationship (Fig. 4) is obtained concerning to an angle of a rear hand side in which each piece starts to rotate when inserted into a predetermined wound tube area.

[0030] wire-stranded hollow tube ($\phi 0.43$) < Ni-Ti wire ($\phi 0.43$) < straight line wire ($\phi 0.43$) = helical coil spring ($\phi 0.43$)

[0031] With the wire-stranded hollow tube 1 superior in torque response and torque transmissibility, a high torque sensitivity is ensured so that a front end swiftly rotates with a small amount of the torque given to the rear hand side.

[0032] In this instances, the wire-stranded hollow tube 1 has twelve line elements ($\phi 0.085$ mm) wound around a line core ($\phi 0.265$ mm). The line core is withdrawn to form the wire-stranded hollow tube 1 which measures ϕ

0.43 mm in outer diameter.

[0033] The helical coil spring is in a single wound helical spring structure in which a line element (ϕ 0.08 mm) is used to have ϕ 0.43 mm in outer diameter.

[0034] The Ni-Ti wire is solid and shaped in a linear configuration to have ϕ 0.43 mm in outer diameter.

[0035] The straight line wire is of a solid stainless steel rectified to increase its linearity with the use of a bearing, roller or the like.

[0036] The following relationship (Fig. 5) is obtained concerning to a torsional torque of the rear hand side in which each piece starts to rotate when inserted into the predetermined wound tube area. wire-stranded hollow tube (ϕ 0.43) < helical coil spring (ϕ 0.43) < Ni-Ti wire (ϕ 0.43) < straight line wire (ϕ 0.43)

[0037] Due to the high torque sensitivity with the least play permitted between the neighboring elements 1a, 1a, the front end swiftly rotates with a small amount of the torque given to the rear hand side. Since the rear hand side takes many turns for the front end to start rotating in the helical coil spring, the helical coil spring is not well-suited to a practical use as understood from the graphical representation in Fig. 4.

[0038] For the wire-stranded hollow tube 1, a good torque response (linear relationship) is ensured in normal and reverse directions in which no substantial delay is perceived in torque response between the rear hand side and the front end as shown in Figs. 6 and 7.

[0039] For the solid line wire (straight line wire (ϕ 0.43) and Ni-Ti wire (ϕ 0.43)), a certain delay can be perceived in the follow-on capability. This tendency is remarkable for the Ni-Ti wire (ϕ 0.43).

[0040] The difference of these characteristics depends on whether the counterpart piece has a hollow flexible structure or a solid rigidity structure. The wire-stranded hollow tube 1 is rendered into the hollow flexible structure so that the aforementioned torque response and torque transmissibility are surmised to be improved albeit the total bending angle increases with a decrease of torsion-resistant moment and rigidity.

[0041] Fig. 8 shows a load efficiency (%) in terms of the total bending angle when a predetermined amount of load (e. g., 50g) is applied to each of the pieces. The graphical representation in Fig. 8 shows the following relationship in the load efficiency. wire-stranded hollow tube (ϕ 0.43) > Ni-Ti wire (ϕ 0.43) > straight line wire (ϕ 0.43)

[0042] This indicates how lightweight the wire-stranded hollow tube is formed with the good manipulatability. The wire-stranded hollow tube 1 superior in torque response and torque transmissibility is well-suited to a medical tube body.

[0043] When the wire-stranded hollow tube 1 is applied to the medical tube body, the medical tube body exhibits a linear torque transmissibility with no significant torque variation. For this reason, the manipulator can advance the medical tube body precisely into a target area of the blood vessel.

[0044] As opposed to the prior art (Figs. 34 and 35) in which the gap (G) is induced at the helical spring (S) to permit an irregular transmissibility and an uneven bending, the wire-stranded hollow tube 1 bends uniformly with a good linear torque transmissibility.

[0045] Fig. 9 shows a medical guide wire 11 in which a core line (hoop line or the like) is inserted into the wire-stranded hollow tube 1 and both ends of the wire-stranded hollow tube 1 is soldered to the core line (not shown).

[0046] Then, an outer surface of the wire-stranded hollow tube 1 is coated with Teflon® (4F) to produce the medical guide wire 11 (usually referred to as "GW"). The same characteristics as the medical tube body has obtained in the previous embodiment are provided with the medical guide wire 11.

[0047] Fig. 10 shows the medical guide wire 11 in which a small tube 11a is fixedly connected to the wire-stranded hollow tube 1. An outer surface of the medical guide wire 11 is coated with a thermoplastic synthetic resin 12 (Teflon®, nylon, polyurethane or the like). On an outer surface of the thermoplastic synthetic resin 12, a hydrophilic polymer 13 (polyvinylpyrrolidone or the like) is coated.

[0048] The thermoplastic synthetic resin 12 may be coated with an inner surface of the medical guide wire 11 or may be coated with both the inner and outer surfaces of the medical guide wire 11. Instead of the thermoplastic synthetic resin 12, a metallic film may be formed by means of sputtering, evaporation or the like. Under the presence of the neighboring elements 1a, 1a twisted, the rear hand side of the medical guide wire 11 appears a convex-concave undulation which prevents a finger slip to enable the manipulator to a firm grip.

[0049] Figs. 11 and 12 show a balloon catheter 14 in which the wire-stranded hollow tube 1 is applied with an inflatable balloon 14a secured to the balloon catheter 14. The wire-stranded hollow tube 1 may be used instead of a hypotube 15. Alternatively, the wire-stranded hollow tube 1 may be used in lieu of a single unit wire 16 placed within the hypotube 15. To the single unit wire 16, a material stipulated in SUS or a Ni-Ti alloy (shape memory alloy) may be employed. The wire-stranded hollow tube 1 may be used to a medical endoscope tube which generally has an identical structure to the medical tube body.

[0050] Fig. 13 shows the wire-stranded hollow tube 1 which is forced to reduce its diameter by means of a die drawing work. Due to the die drawing work, the neighboring elements 1a, 1a of the metal wires 8 deforms to tightly engage each other so as to produce a good circularity with a uniform diameter substantially maintained. The die drawing work increases a contact pressure between the neighboring elements 1a, 1a to tightly unite the neighboring elements 1a, 1a to produce a quick torque response and a good torque transmissibility. When the wire-stranded hollow tube 1 is used to the balloon catheter, a good pushability is further ensured.

[0051] Fig. 14 shows a wire-stranded hollow tube 18 in which a stainless steel wire 20 and a Ni-Ti alloy wire 21 are stranded alternately to serve as different metallic wires.

[0052] When the wire-stranded hollow tube 18 is forced to reduce its diametrical dimension by a compression shrinkage (Δt) with the use of the swaging or the die drawing work as shown in Fig. 15, the hard Ni-Ti alloy wire 21 tightly engages against the stainless steel wire 20 to deform the stainless steel wire 20. This makes the Ni-Ti alloy wire 21 contact with the stainless steel wire 20 with an increased contact area to tightly unite them together to achieve a more improved torque transmissibility.

[0053] Fig. 16 shows a second embodiment of the invention in which the wire-stranded hollow tube 1 is applied to the medical guide wire 11. To the wire-stranded hollow tube 1, an elongated core 22 is inserted, an outer diameter of which is slightly smaller than an inner diameter of the wire-stranded hollow tube 1. Both ends of the wire-stranded hollow tube 1 are soldered to the elongated core 22.

[0054] In this instance, the medical guide wire 11 is effective in particular when a pushability is needed in addition to a quick torque response. In this situation, the elongated core 22 may be in a solid or hollow configuration.

[0055] Figs. 17 ~ 21 show a third embodiment of the invention in which a wire-stranded hollow tube 32 is applied to the medical guide wire 30. The medical guide wire 30 has the wire-stranded hollow tube 32 formed relatively longer by twisting many turns a plurality (e.g., 12) of metallic wires 32a, and having an elastic elongation core 34 which progressively decreases its diametrical dimension toward a front end of the elongation core 34. A synthetic resin tube 36 is fixed around the elongation core 34 except for a tapered-off portion of the elongation core 34. A front helical spring 38 is secured to surround the tapered-off portion of the elongation core 34.

[0056] As a basal side resin layer, an outer surface of the wire-stranded hollow tube 32 is coated with a fluoride-based resin layer (not shown) such as, for example, a polytetrafluoroethylene layer (PTFE), a thickness of which is approx. 8 μ m. In order to provide a smoothness and a thrombus-repellant property, the basal side resin layer is formed by a hydrophobic synthetic resin such as a silicone resin in addition to the fluoride-based resin layer.

[0057] In the elongation core 34 located in a hollow portion 32b of the wire-stranded hollow tube 32, a basal end of the wire-stranded hollow tube 32 is plasma welded to a basal main body 34a together with a rear tip 35. A front end of the wire-stranded hollow tube 32 is soldered to the elongation core 34. As a material of the elongation core 34, used are a stainless steel, a piano wire and superelastic metals such as Ni-Ti alloy, Cu-Zn-Q alloy (Q = Al, Fe or the like), Ni-Ti-Q alloy (Q = Cu, Fe, V, Co or the like).

[0058] The synthetic resin tube 36 provides a flexibility with an outer extension 34b of the elongation core 34, and at the same time, protecting an area in which the synthetic resin tube 36 covers. By way of illustration, the synthetic resin tube 36 is formed by polyurethane, polyvinylchloride, polyester or the like. To the synthetic resin tube 36, a required amount of powder prescribed from barium sulfate, bismuth, tungsten or the like is added as an X-ray impervious agent. Coated with an outer surface of the synthetic resin tube 36 is a hydrophobic resin film 37 formed by polyvinylpyrrolidone (PVP), polyethylene glycol or the like in order to further provide the smoothness and the thrombus-repellent property.

[0059] A front helical spring 38 is secured to surround a leading end of the outer extension 34b, and fixed to the outer extension 34b by means of a soldering or an adhesive. The front helical spring 38 at least partly contains the X-ray impervious agent such as silver, platinum, bismuth, tungsten, Pt-Ni alloy or the like.

[0060] Figs. 22 ~ 24 show a fourth embodiment of the invention. The fourth embodiment of the invention differs from the third embodiment of the invention in that instead of the synthetic resin tube 36 and the front helical spring 38, a continuous helical spring 39a formed with a stainless steel is secured to surround the outer extension 34b of the elongation core 34.

[0061] In this instance, a metallic wire (ϕ 0.17 mm in dia.) which is formed by the material stipulated in SUS 304 is used to the wire-stranded hollow tube 32. A metallic wire (ϕ 0.40 mm in dia.) which is formed by the material stipulated in SUS 304 is used to the elongation core 34. An equi-diametrical portion (ϕ 0.10 mm in dia.) resides at a front extension area (5.0 mm) of the elongation core 34. A metallic wire (ϕ 0.15 mm in dia.) which is formed by the material stipulated in SUS 304 is used to the continuous helical spring 39a which measures 0.89 mm in outer diameter.

[0062] The wire-stranded hollow tube 32 is soldered to the continuous helical spring 39a together with the elongation core 34 at their common junction 40. The continuous helical spring 39a is also bonded to the outer extension 34b of the elongation core 34 at a designated middle portion 41. Coated with outer surfaces of the wire-stranded hollow tube 32 and the continuous helical spring 39a are a synthetic resin layer (PTFE) 42, a thickness of which measures approx. 8 μ m. On an outer surface of the synthetic resin layer 42, a hydrophobic resin film 43 is formed.

[0063] With the continuous helical spring 39a connected in series with the wire-stranded hollow tube 32, a good flexibility is provided with the medical guide wire 30, thus enabling the manipulator to effectively advance deep into the wound and small blood vessel by staunchly following on the wound and small configuration at the time of inserting the medical guide wire 30 into the serpentine blood vessel.

[0064] Fig. 25 shows a fifth embodiment of the invention. In the fifth embodiment of the invention, a semicon-

ductor type pressure sensor 44 is provided to measure a blood pressure value at front and rear portions of a stricture area of the blood vessel by inserting the medical guide wire 30 to reopen an obstructive coronary artery at the time of conducting a percutaneous transluminal coronary angioplasty (PTCA). Instead of the rear tip 35 of Fig. 22, the pressure sensor 44 is placed within a metallic tube 45 which is bonded to the wire-stranded hollow tube 32 by means of a soldering or the like. A microcable 46 (microwire connection) is stretched along an inner space of the medical guide wire 30.

[0065] Fig. 26 shows a sixth embodiment of the invention. In the sixth embodiment of the invention, the pressure sensor 44 is installed into the metallic tube 45. The wire-stranded hollow tube 32 is divided into a front majority piece 32A and a rear minor piece 32B, and the metallic tube 45 is provided between the front majority piece 32A and the rear minor piece 32B. Front and rear ends of the metallic tube 45 form the respective diameter-reduced tube connectors 45a, 45b. The diameter-reduced tube connectors 45a, 45b are connected and soldered to the front majority piece 32A and the rear minor piece 32B.

[0066] Fig. 27 shows a seventh embodiment of the invention. In the seventh embodiment of the invention, a short helical spring 47 which contains the radiation-imperious agent (radiopaque agent) is provided instead of the rear minor piece 32B of Fig. 26.

[0067] In the fifth through seventh embodiments, the pressure sensor 44 is provided with the medical guide wire 30 to measure the blood pressure from the following reasons.

[0068] As a conventional medical guide wire, a medical tube 50 has been used in which a metallic wire net is covered with a synthetic resin coat, otherwise a synthetic resin is formed into tubular configuration. Upon inserting the medical tube 50 into a wound and small blood vessel 51 as shown in Fig. 28, the medical tube 50 is subjected to deformation due to torsion, distortion and bending when inserting the medical tube 50 into a wound portion of the blood vessel 51. When the medical tube 50 is subjected to the deformation, a precise blood pressure measurement and monitoring are rendered unable during the manipulating the medical tube 50 for an extended period of time.

[0069] This is because the medical tube 50 is supposed to deform substantially flat to be elliptic in cross section as shown in Fig. 29. When the medical tube 50 deforms flat, blood paths 52, 53 vary its cross section between the medical tube 50 and an inner wall 51a of the blood vessel 51. The narrower blood path 52 allows blood streams to flow quickly, and the wider blood path 53 allows blood streams to flow slowly. Due to the difference of the blood stream velocity between the blood paths 52, 53, the blood stream is disturbed to fluctuate the blood pressure value measured by the pressure sensor. This tendency becomes more remarkable as the blood vessel becomes smaller. The situation renders

the medical tube 50 unable to cope with the blood pressure measurement for the obstructive coronary artery.

[0070] On the contrary, the medical guide wire 30 according to the fifth through seventh embodiments enables the manipulator to use it smoothly in the wound and small coronary artery (1~3 mm), and thus ensuring a precise blood pressure measurement and monitoring during manipulating the medical guide wire 30 for an extended period of time.

[0071] This is surmisably because the medical guide wire 30 generally maintains a circular shape stable in cross section (Fig. 32) without deforming flat at a wound portion of a wound and small blood vessel 54 when inserting the medical guide wire 30 into the wound and small blood vessel 54 as shown in Fig. 30. Namely, the metallic wires 32a are each twisted to form the wire-stranded hollow tube 32 so that each metallic wire 32a relatively slides slightly along its helical line when the wire-stranded hollow tube 32 is bent. This keeps a tight engagement between the metallic wires 32a to generally maintain the circular shape stable in cross section as opposed to a single wound helical spring 55 which produces a gap (Sp) between the line elements 55a as mentioned hereinafter.

[0072] The single wound helical spring 55 produces the gap (Sp) between the line elements 55a at the wound portion when the single wound helical spring 55 is bent as shown in Fig. 31, although the single wound helical spring 55 substantially maintains a circular shape in cross section without deforming flat at the wound portion. The gap (Sp) appeared between the line elements 55a causes a turbulence in the blood streams to fluctuate the blood pressure value measured by the pressure sensor.

[0073] In the medical guide wire 30, the wire-stranded hollow tube 32 only allows the metallic wires 32a to slightly slide along the helical line while maintaining the tight engagement between the metallic wires 32a to generally keep the circular shape stable in cross section without producing the gap between the metallic wires 32a as shown in Fig. 32. This resultantly generates no significant difference in the blood path between the medical guide wire 30 and the inner wall of the blood vessel to induce no significant turbulence in the blood streams, and thereby enabling the manipulator to the precise blood pressure measurement and monitoring for an extended period of time.

[0074] Due to helical grooves appeared between the metallic wires 32a, the blood streams are smoothly guided along the helical grooves to induce no significant fluctuation in the blood pressure value measured by the pressure sensor 44.

[0075] When the single wound helical spring 55 is bent as shown in Fig. 33, the single wound helical spring 55 is expanded at its outer tensile side. This stretches the single wound helical spring 55 to make its axial length (Lb) longer than the original length (La). The axial length (La) stretches more remarkable as the single

wound helical spring 55 is bent deeper. For this reason, the microcable of the pressure sensor 44 is feared to be snapped off due to a sufficient tensile force subjected to the microcable especially when advancing the single wound helical spring 55 into a deeply wound portion of the wound and small blood vessel 54.

[0076] In the medical guide wire 30 into which the wire-stranded hollow tube 32 is incorporated, the metallic wires 32a slightly slide each other to maintain the tight engagement therebetween without being expanded at the outer tensile side when the wire-stranded hollow tube 32 is deeply bent. This remains the axial length of the wire-stranded hollow tube 32 substantially unchanged. There is no fear that the microwire connection 46 is snapped off because no sufficient tensile force is subjected to the microcable 46 when advancing the medical guide wire 30 into the deeply wound portion of the wound and small blood vessel. The medical guide wire 30 is resultantly well-suited particularly when used to advance into an acutely wound portion of the wound and small blood vessel.

[0077] It is to be noted that outer surfaces of the wire-stranded hollow tube 32 and the short helical spring 47 are each coated with the synthetic resin layer over which the hydrophilic resin film is coated, although not shown.

(a) The medical tube body and the medical guide wire may have a plurality (e.g., 2 ~ 3) of wire-stranded hollow tubes concentrically arranged to form a multilayered configuration.

(b) In the wire-stranded hollow tube, the metallic wire may be not only circular but also rectangular, triangular, pentagonal, hexagonal, polygonal and elliptic in cross section.

(c) The metallic wires of different helical pitch may be used to produce a tighter engagement between the neighboring metallic elements by providing the wire-stranded hollow tube with a strengthened compression.

(d) In general, the medical guide wire is 0.35~1.0 mm in outer diameter and the medical tube body is 0.4 ~ 3.0 mm in outer diameter, however these outer diameters are not confined merely to these statistics.

Claims

1. A wire-stranded hollow tube comprising:

a plurality of metallic wires preformed with a predetermined forming rate being twisted along a circular line and postformed in order to provide a good circularity and diametrical uniformity so as to be rendered thereafter to be coreless hollow configuration.

2. The wire-stranded hollow tube according to claim

1, wherein said forming rate which preforms said metallic wires is within a range of 90% to 98%.

3. The wire-stranded hollow tube according to claim 1 or 2, wherein said plurality of metallic wires comprises at least two wires made from different materials from each other.

4. A medical tube body formed by the wire-stranded hollow tube according to any one of claims 1 to 3.

5. A medical guide wire formed by the wire-twisted hollow tube according to any one of claims 1 to 4.

6. A medical guide wire comprising:

a wire-stranded hollow tube formed by a plurality of metallic wires twisted along a circular line to be shaped into a coreless hollow configuration;

a single elastic elongation core inserted into a hollow portion of said wire-stranded hollow tube, and having a basal main body located within said wire-stranded hollow tube, and further having an outer extension which is diametrically smaller than said basal main body and extends beyond a front end of said wire-stranded hollow tube by a predetermined length; and a synthetic resin layer coated with an outer surface of said outer extension of said elongation core by its predetermined axial length.

7. A medical guide wire comprising:

a wire-stranded hollow tube formed by a plurality of metallic wires twisted along a circular line to be shaped into a coreless hollow configuration;

a single elastic elongation core inserted into a hollow portion of said wire-stranded hollow tube, and having a basal main body located within said wire-stranded hollow tube, and further having an outer extension which is diametrically smaller than said basal main body and extends beyond a front end of said wire-stranded hollow tube by a predetermined length; and a metallic helical spring wound around said outer extension of said elongation core by its entire axial length.

8. The medical guide wire according to claim 7, wherein said metallic helical spring at least partially contains a radiation-impervious agent.

9. The wire-stranded hollow tube, medical tube body and medical guide wire according to any one of claims 1 to 8, which is subjected to a diameter-reduction such as a swaging or a die drawing work.

10. The wire-stranded hollow tube, the medical tube body and the medical guide wire according to any one of claims 1 to 8, wherein a plurality of said wire-stranded hollow tubes are concentrically arranged to form a multilayered configuration.

5

11. The medical guide wire according to any one of claims 5 to 8, wherein a pressure sensor is provided to measure a blood pressure when inserted into a human blood vessel.

10

15

20

25

30

35

40

45

50

55

Fig. 1

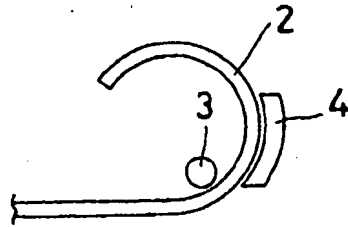


Fig. 1a

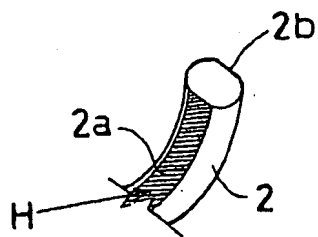


Fig. 1b

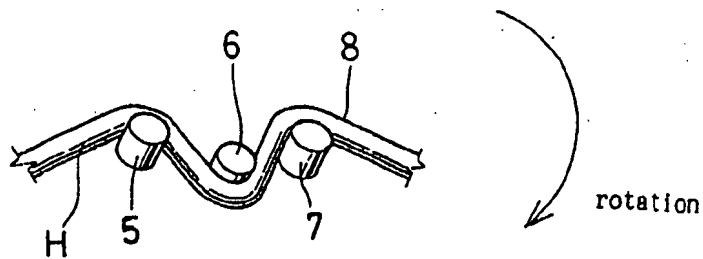


Fig. 1c




Fig. 2

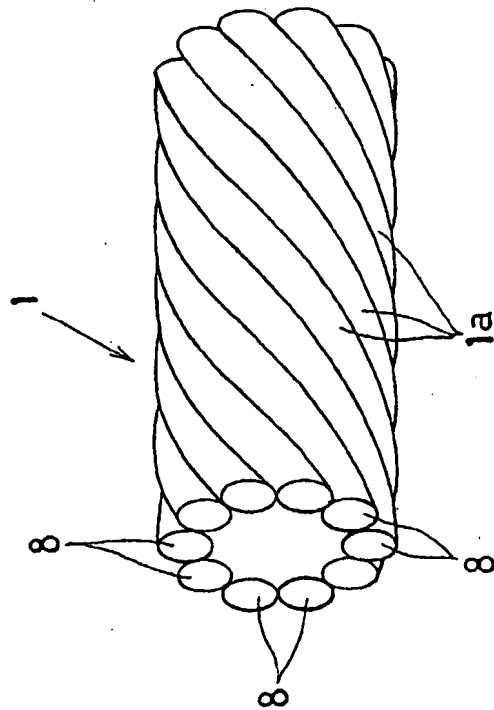


Fig. 3

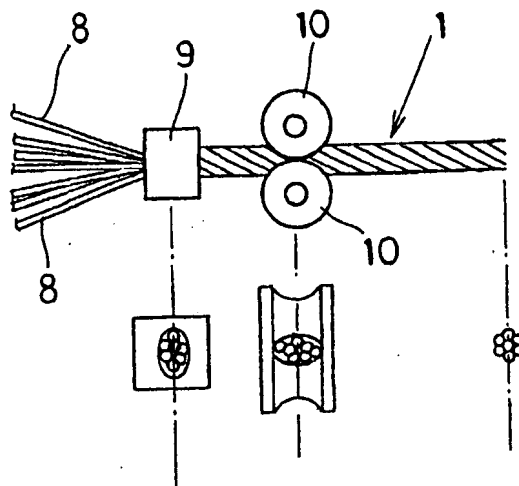


Fig. 4

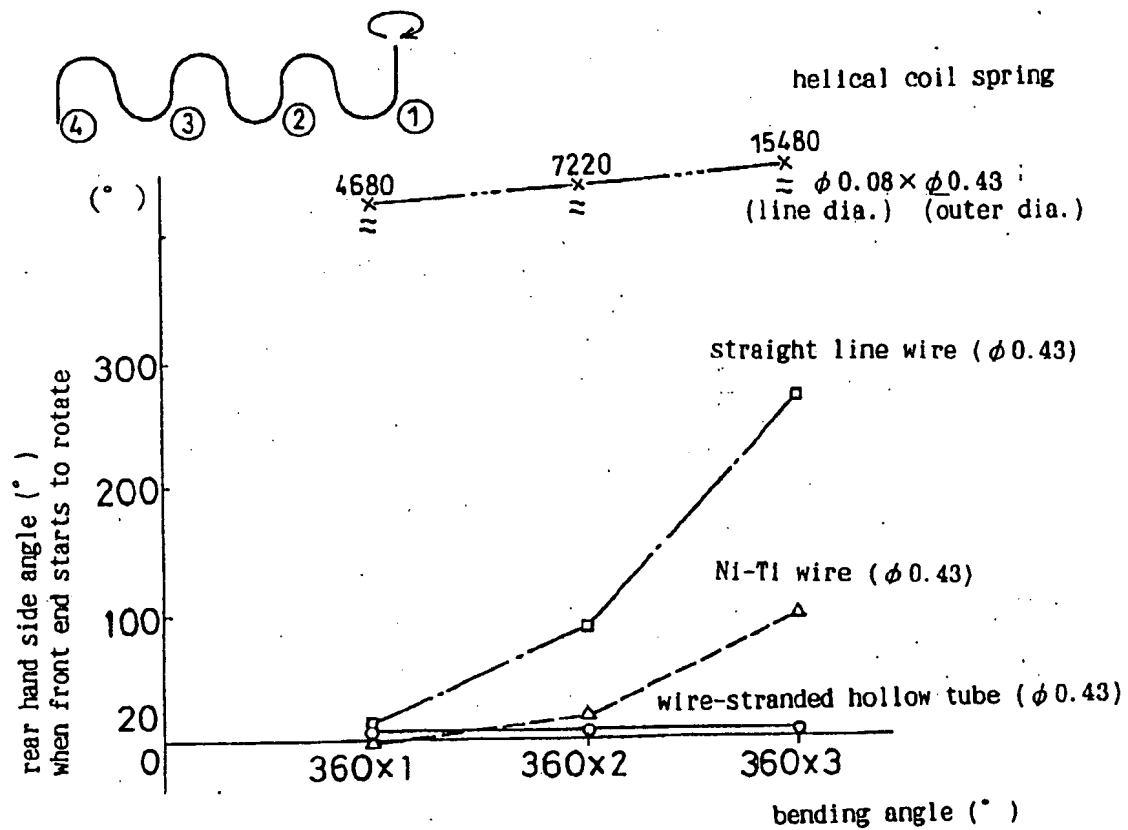


Fig.5

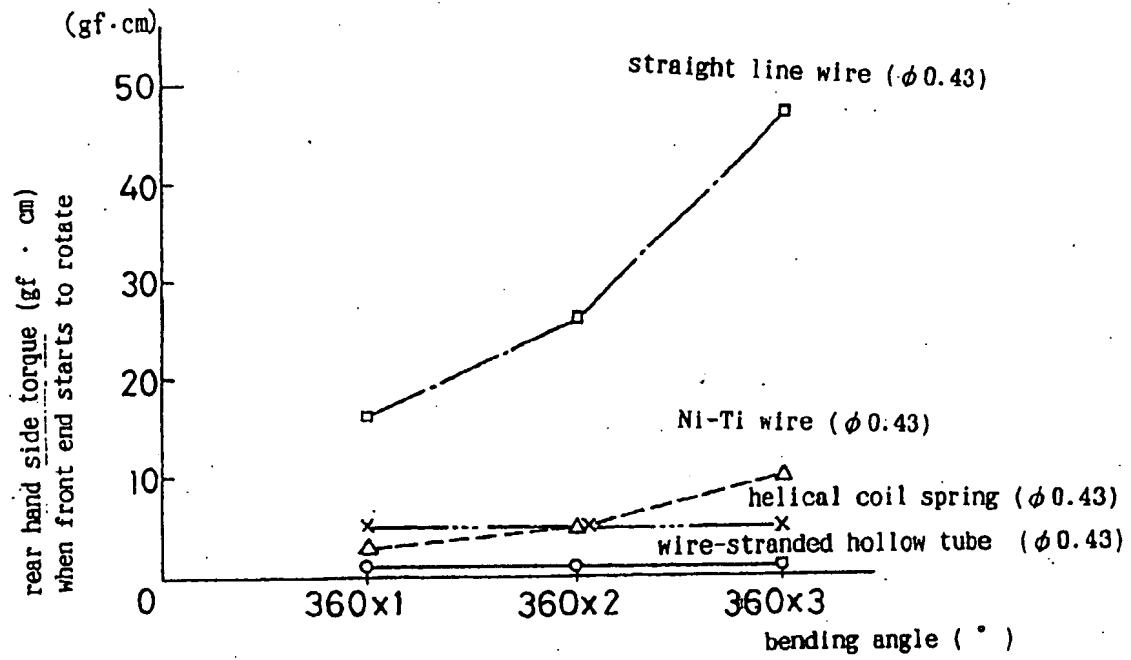


Fig.6

normally directed rotation

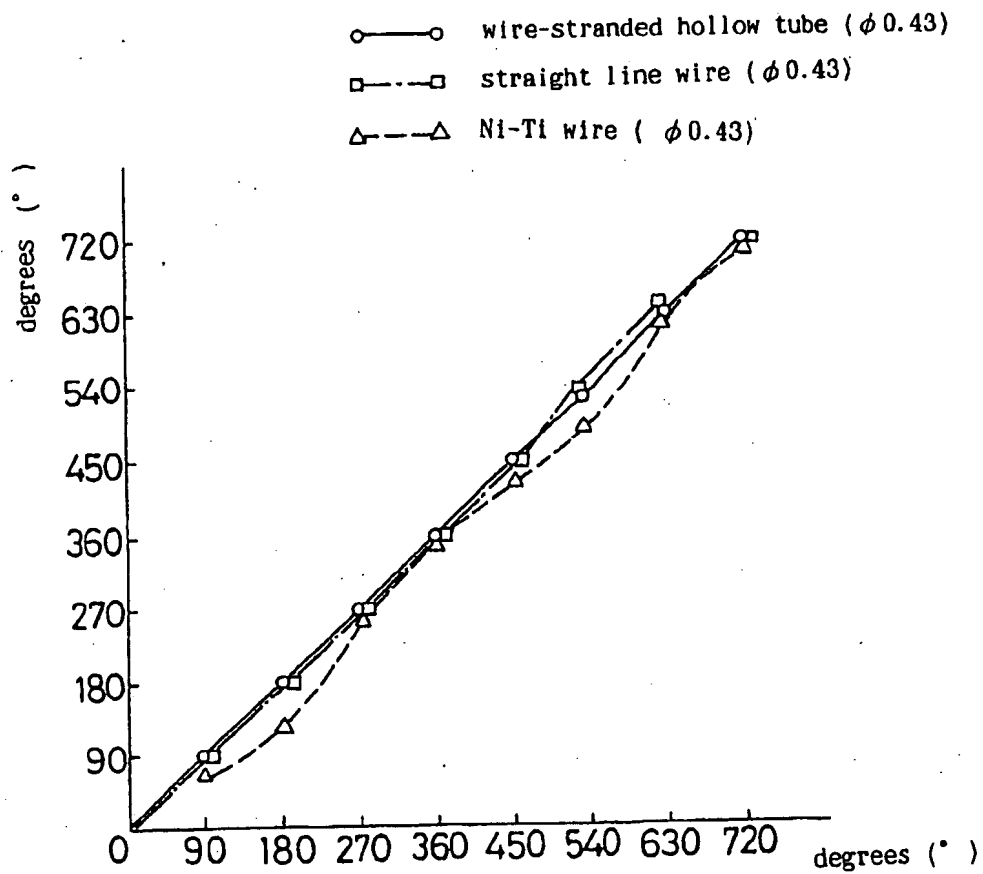


Fig.7

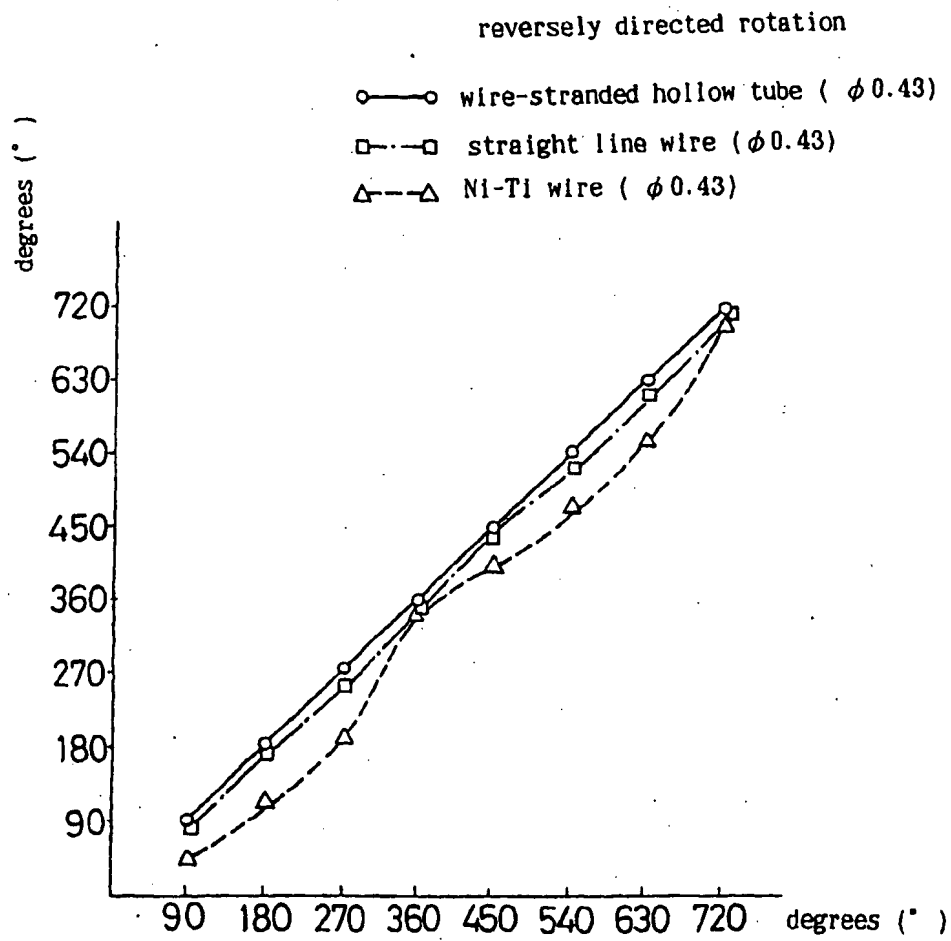


Fig. 8

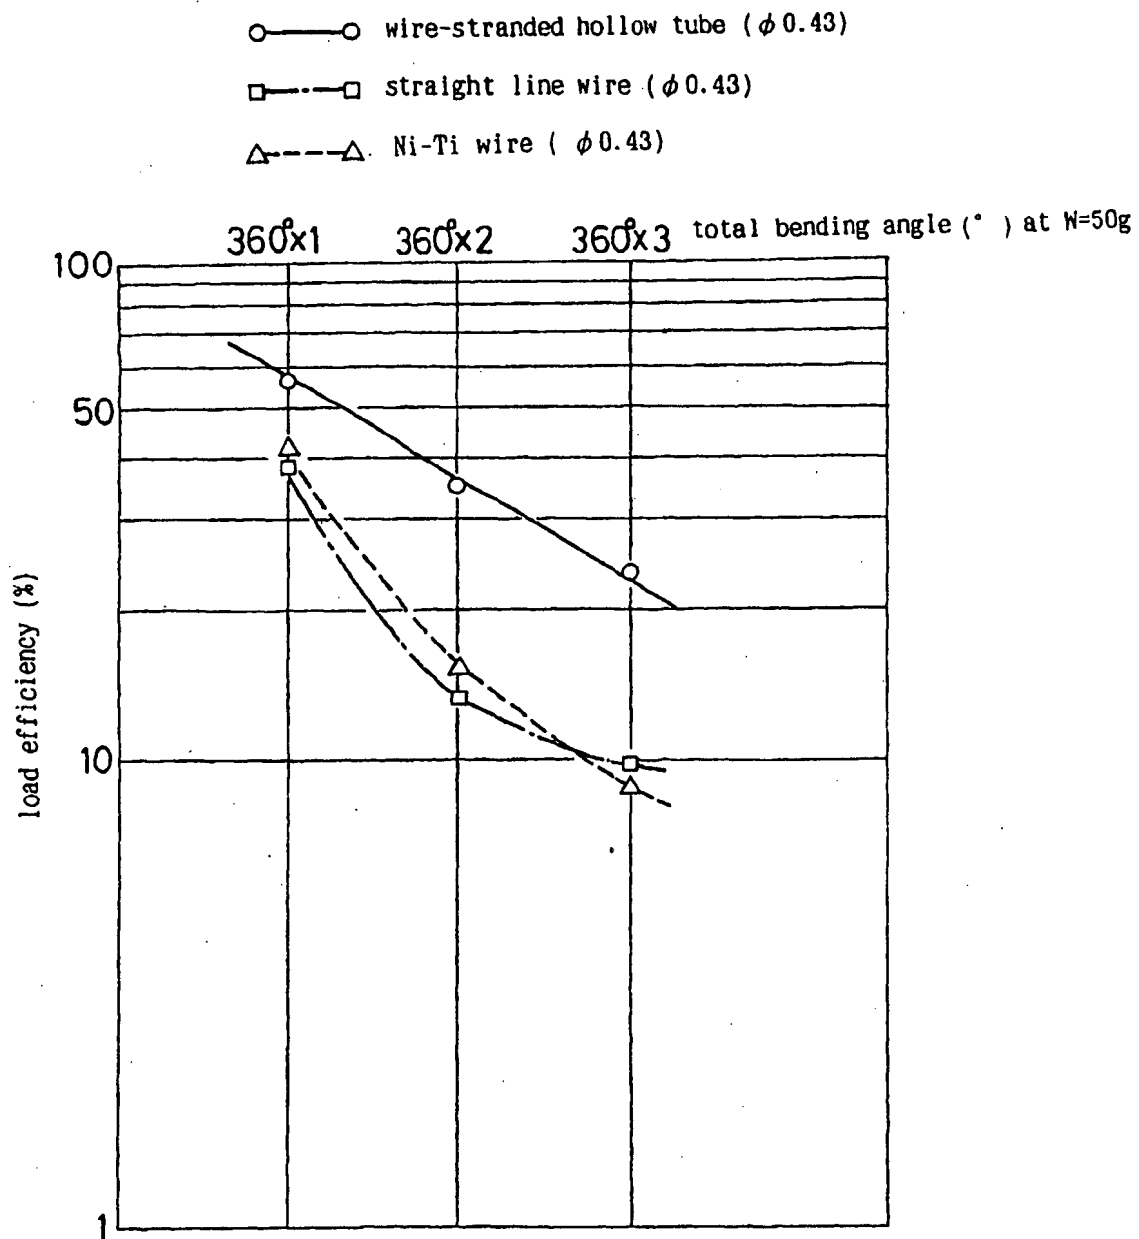
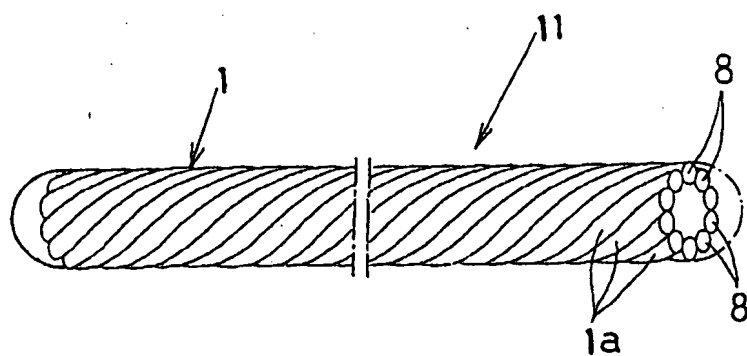


Fig. 9



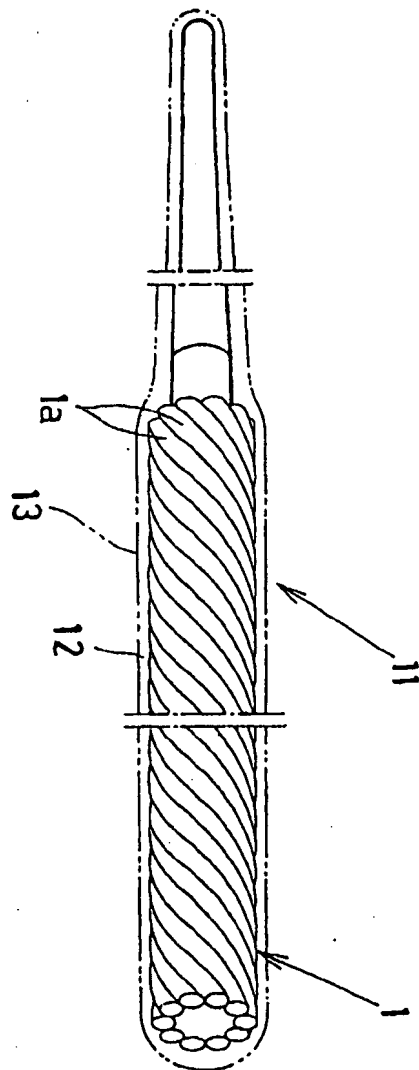


Fig. 10

Fig. 11

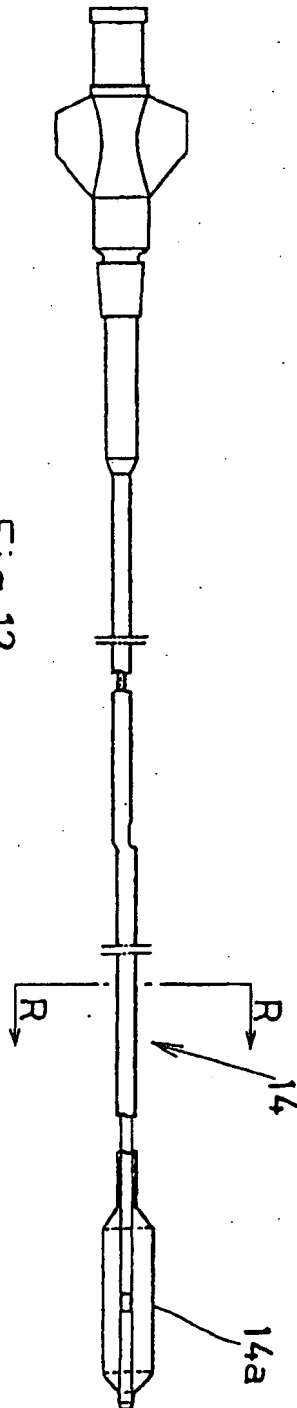



Fig. 12



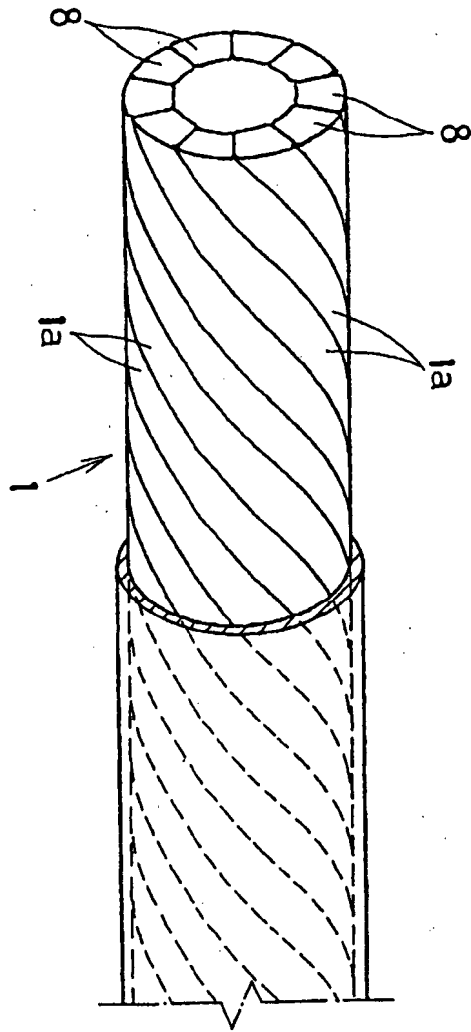


Fig.13

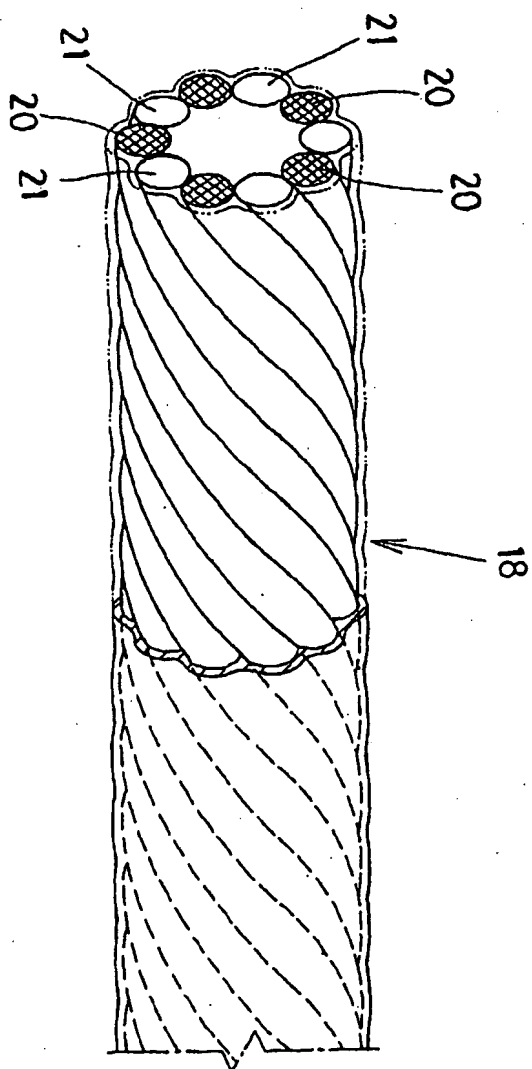
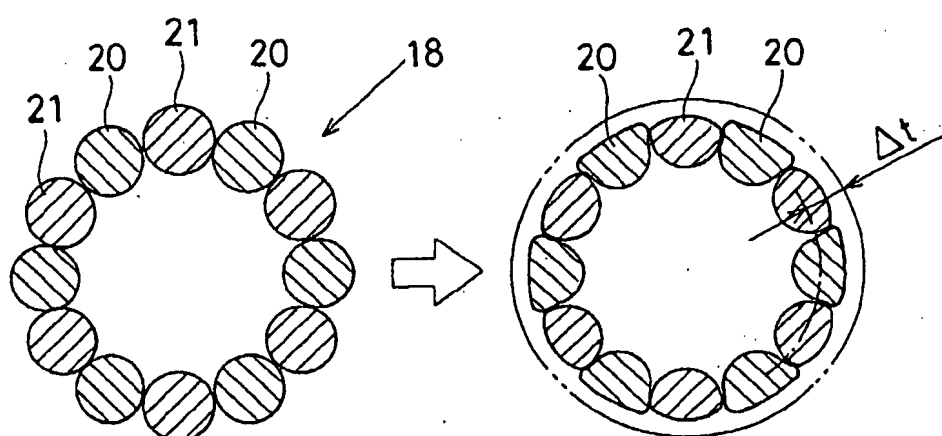


Fig. 14

Fig. 15



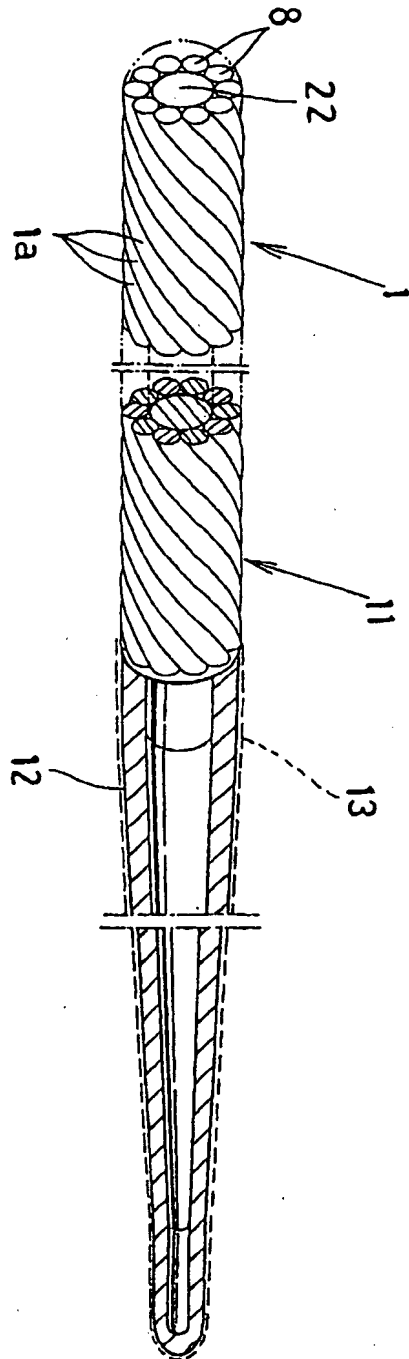


Fig. 16

Fig.17

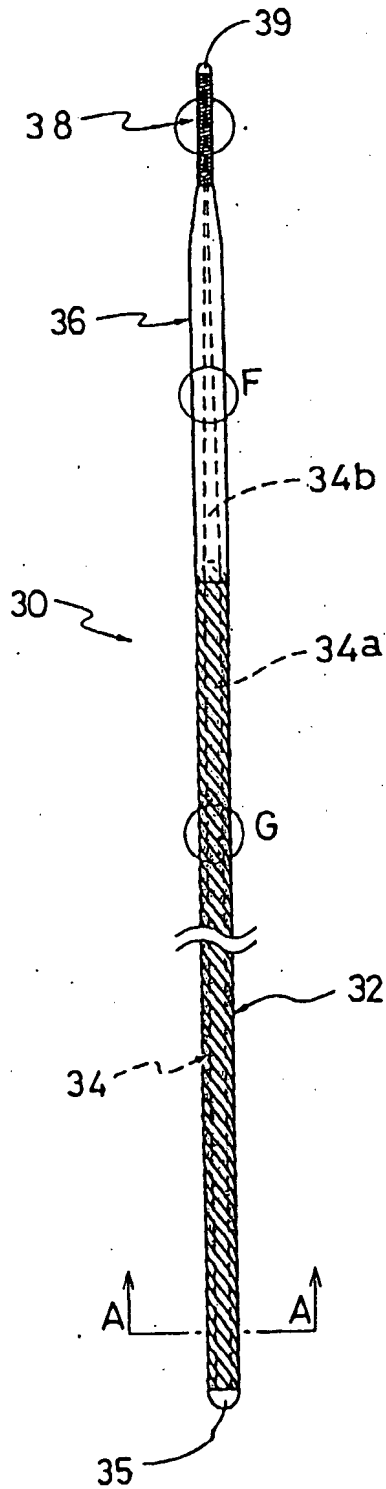


Fig.18

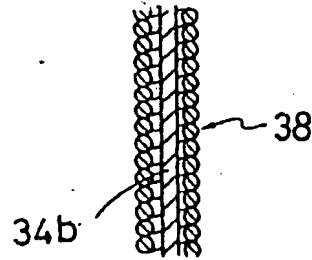


Fig.19

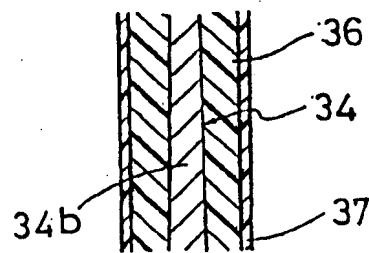


Fig. 20

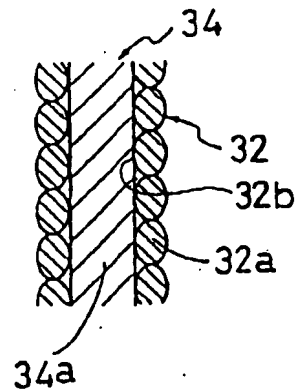
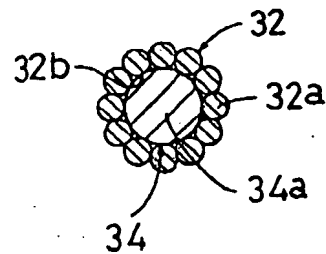


Fig. 21



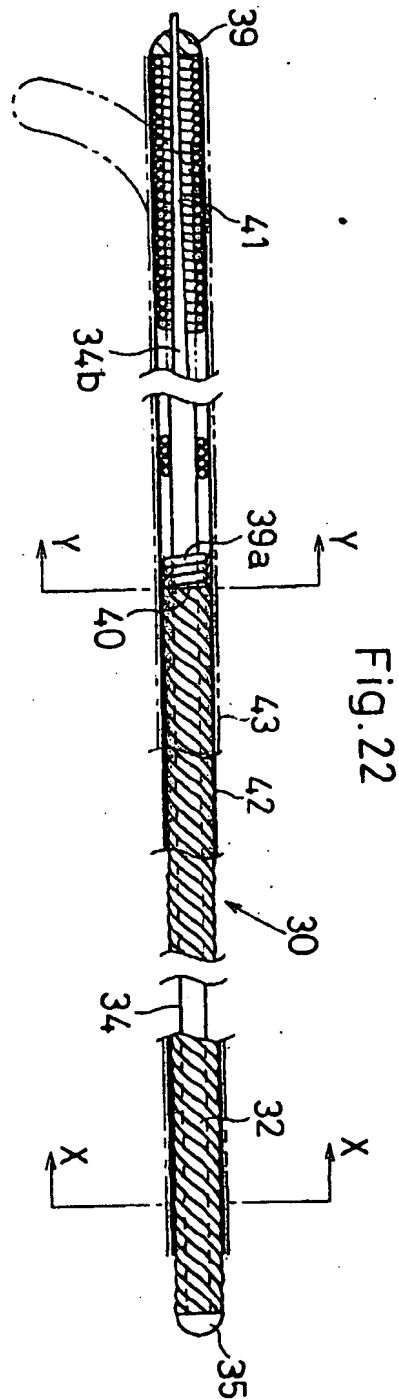


Fig. 22

Fig. 23





Fig. 24



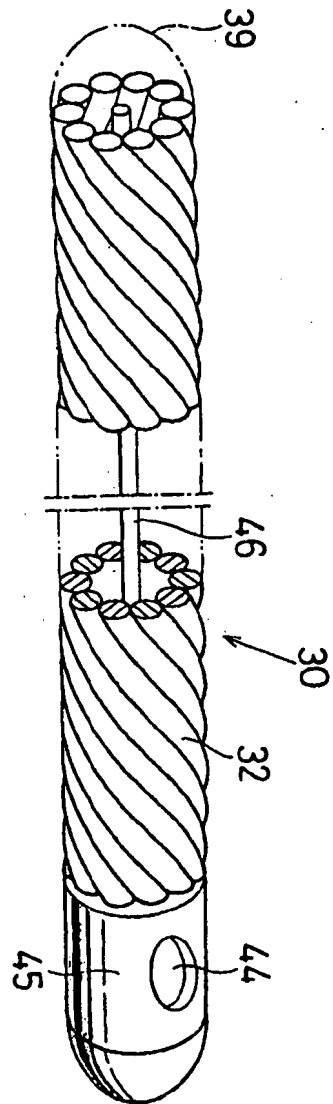
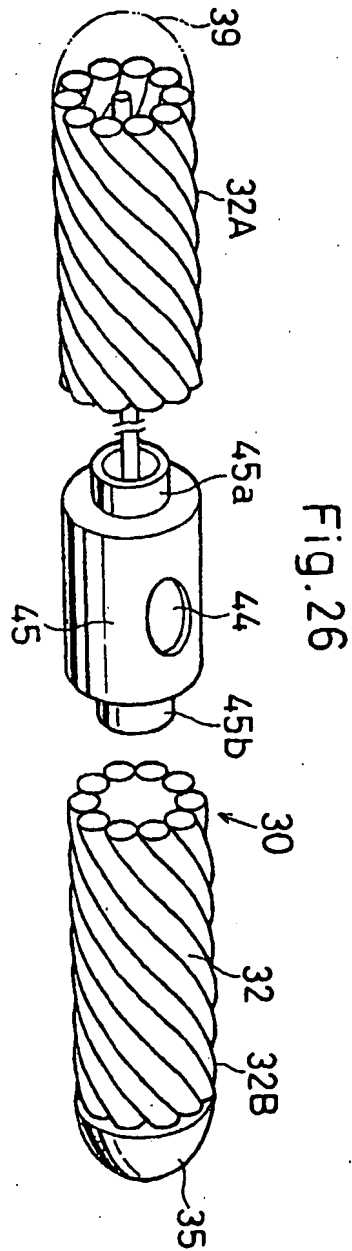


Fig. 25



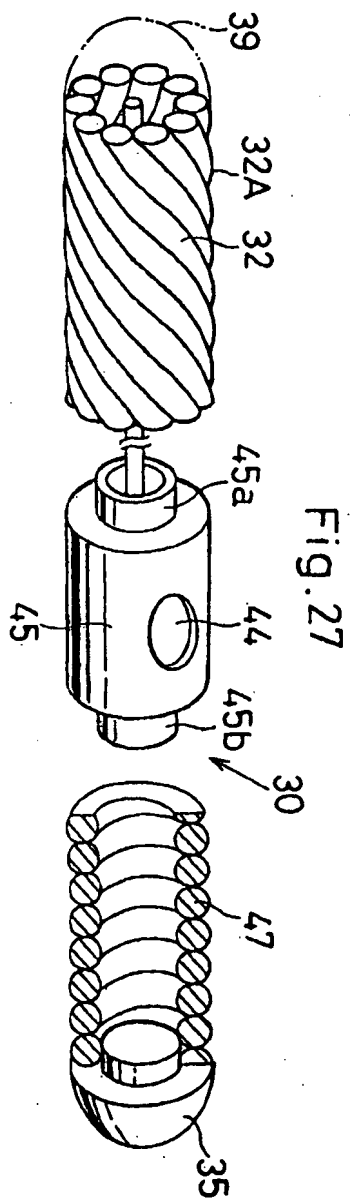


Fig. 28

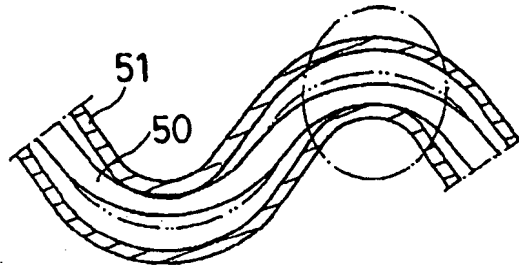


Fig. 29

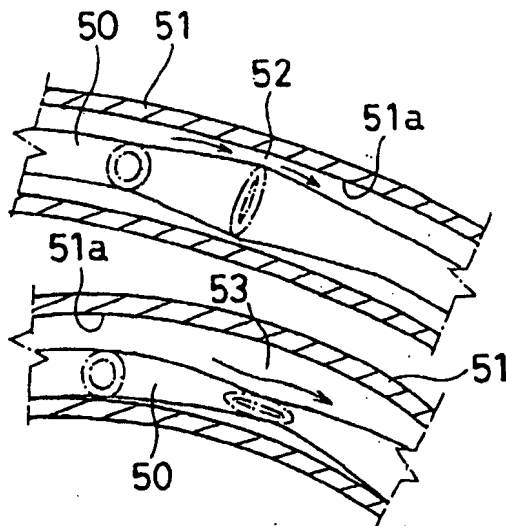


Fig. 30

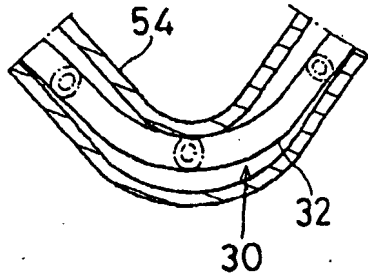


Fig. 31

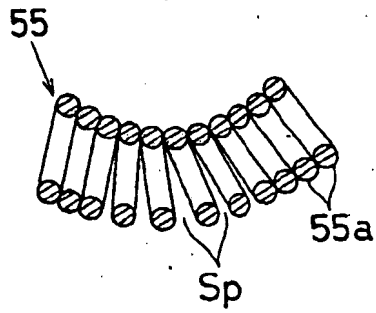


Fig. 32


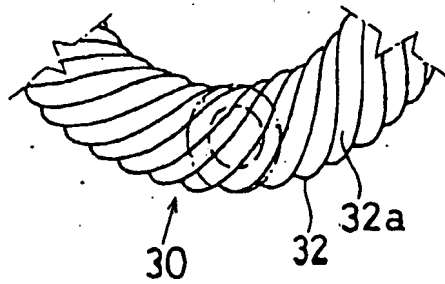


Fig. 33

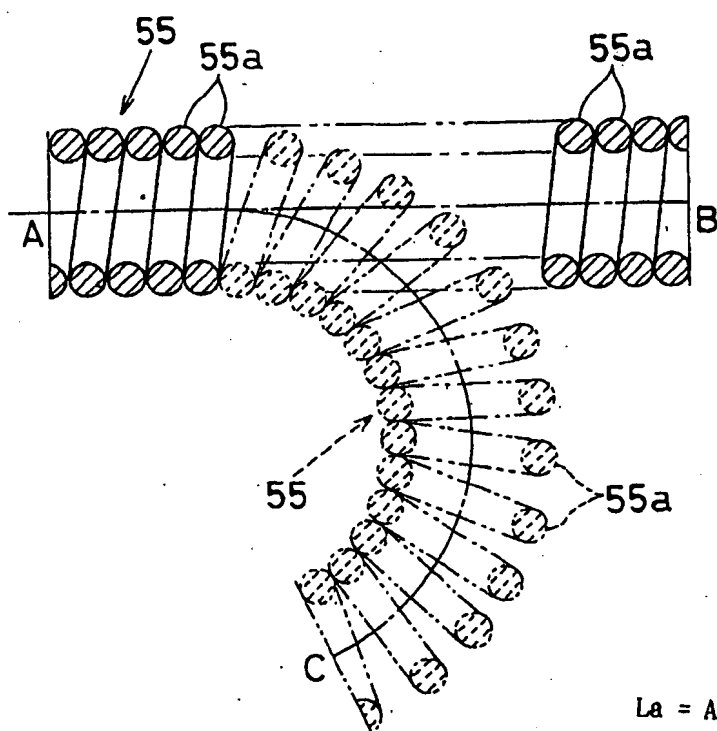

$$L_a = AB$$

$$L_b = AC$$

$$L_a < L_b$$

Fig. 34


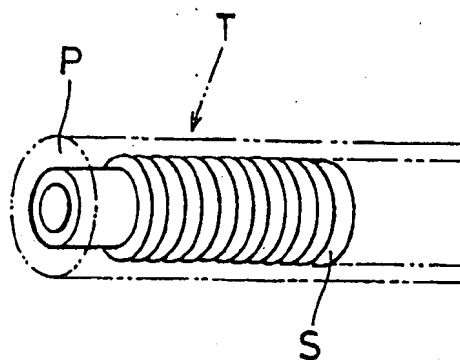


Fig. 35



(19)

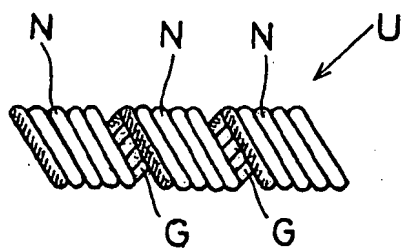

Europäisches Patentamt

European Patent Office

Office européen des brevets



(11)

EP 1 243 283 A3

(12)

EUROPEAN PATENT APPLICATION

(88) Date of publication A3:

04.06.2003 Bulletin 2003/23

(51) Int Cl.7: **A61M 25/00, A61M 25/01**

(43) Date of publication A2:

25.09.2002 Bulletin 2002/39

(21) Application number: **02251981.3**(22) Date of filing: **20.03.2002**

(84) Designated Contracting States:

**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR**

Designated Extension States:

AL LT LV MK RO SI(30) Priority: **21.03.2001 JP 2001081416****10.08.2001 JP 2001243937**(71) Applicant: **ASAHI INTECC CO., LTD.****Nagoya-shi, Aichi-ken (JP)**

(72) Inventors:

- Miyata, Naohiko, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Kato, Tomihisa, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)
- Miyata, Kenji, c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)

• Osawa, Toshiya c/o ASAHI INTECC CO.LTD., Nagoya-shi, Aichi-ken (JP)


• Matsuo, Kazumi c/c ASAHI INTECC CO LTD., Nagoya-shi, Aichi-ken (JP)

• Kusuda, Ryuji c/o ASAHI INTECC CO LTD., Nagoya-shi, Aichi-ken (JP)

• Nakagoshi, Yoshinobu
c/o ASAHI INTECC CO.LTD.,
Nagoya-shi, Aichi-ken (JP)• Kato, Tadakazu c/o ASAHI INTECC CO.LTD.,
Nagoya-shi, Aichi-ken (JP)(74) Representative: **Senior, Alan Murray****J.A. KEMP & CO.,****14 South Square,****Gray's Inn****London WC1R 5JJ (GB)**(54) **A wire-stranded hollow tube, a medical tube body and a medical guide wire**

(57) In a wire-stranded hollow tube 1, a plurality of metallic wires (8) preformed with a predetermined forming rate are twisted along a circular line into a coreless hollow configuration. When twisting the metallic wires (8), the neighboring metallic elements (1a, 1a) are subjected to compression with no gap appeared between the neighboring metallic elements (1a, 1a). This increases a contact pressure between the neighboring metallic elements (1a, 1a) to attain a good tightness with a good circularity and diametrical uniformity, and thereby preventing the wire-stranded hollow tube 1 from inadvertently collapsing. A tightness is strengthened between the neighboring metallic elements (1a, 1a) when the metallic elements (1a, 1a) of different helical pitch are used. By applying the wire-stranded hollow tube 1 to a medical guide wire, a quick torque response and a good torque transmissibility are ensured which leads to a good manipulatability with a favorable follow-on capability.

Fig. 2

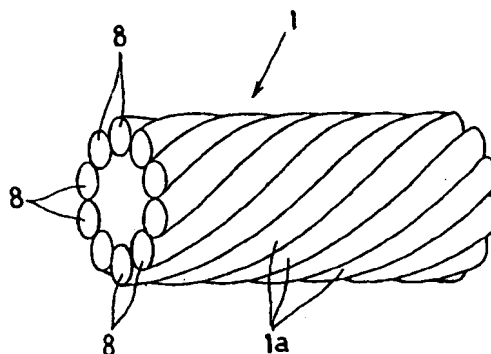

EP 1 243 283 A3



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 02 25 1981

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
X	US 4 579 127 A (HAACKE CLAUS) 1 April 1986 (1986-04-01)	1,2,4,5	A61M25/00 A61M25/01
Y	* the whole document *	6	
Y	---		
Y	EP 0 826 389 A (ASAHI INTECC CO LTD) 4 March 1998 (1998-03-04)	6	
A	* claim 1; figures *	1,2,4,5	
X	---		
X	EP 1 040 843 A (COOK WILLIAM EUROP ; COOK INC (US)) 4 October 2000 (2000-10-04) * column 5, line 30 - column 6, line 55 * * column 7, line 27 - line 33; figures *	1-5,9,10	
A	---		
A	EP 0 200 919 A (INTERMEDICAT GMBH) 12 November 1986 (1986-11-12) * page 7, line 17 - line 28; figures *	1,2,4-6	
A	---		
A	WO 96 07351 A (CARDIOMETRICS INC) 14 March 1996 (1996-03-14) * abstract; figures *	11	

			TECHNICAL FIELDS SEARCHED (Int.Cl.7)
			A61M
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 10 December 2002	Examiner KOUSOURETAS, I
CATEGORY OF CITED DOCUMENTS		I : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons A : member of the same patent family, corresponding document	
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document			

EPO FORM 1503 03/82 (P04C01)



European Patent
Office

Application Number
EP 02 25 1981

CLAIMS INCURRING FEES

The present European patent application comprised at the time of filing more than ten claims.

- ☐ Only part of the claims have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims and for those claims for which claims fees have been paid, namely claim(s):
- ☐ No claims fees have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims.

LACK OF UNITY OF INVENTION

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

see sheet B

- ☐ All further search fees have been paid within the fixed time limit. The present European search report has been drawn up for all claims.
- ☐ As all searchable claims could be searched without effort justifying an additional fee, the Search Division did not invite payment of any additional fee.
- ☐ Only part of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the inventions in respect of which search fees have been paid, namely claims:
- ☒ None of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims, namely claims:

1-6, 9-11



European Patent
Office

LACK OF UNITY OF INVENTION
SHEET B

Application Number

EP 02 25 1981

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

1. Claims: 1-6,9-11

A medical guidewire comprising a wire-stranded hollow tube formed by a plurality of metallic wires twisted along a circular line, a single elongation core inserted into a hollow portion of said tube and having an extension which extends beyond a front end of said tube and a synthetic resin layer coated with an outer surface of the extension of the elongation core.

2. Claims: 7-11

A medical guidewire comprising a wire-stranded hollow tube formed by a plurality of metallic wires twisted along a circular line, a single elongation core inserted into a hollow portion of said tube and having an extension which extends beyond a front end of said tube and a metallic helical spring wound around said outer extension of the elongation core.

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 02 25 1981

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

10-12-2002

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 4579127	A	01-04-1986	DE 3327779 A1	14-02-1985
			AT 23116 T	15-11-1986
			DE 3461055 D1	04-12-1986
			EP 0132694 A2	13-02-1985
			ES 280851 U	16-02-1985
			IE 55752 B1	02-01-1991
EP 0826389	A	04-03-1998	JP 10076014 A	24-03-1998
			DE 69707789 D1	06-12-2001
			DE 69707789 T2	02-05-2002
			EP 0826389 A2	04-03-1998
EP 1040843	A	04-10-2000	EP 1040843 A1	04-10-2000
			AU 4328300 A	16-10-2000
			EP 1165170 A1	02-01-2002
			JP 2002539901 T	26-11-2002
			WO 0057944 A1	05-10-2000
			US 2002074051 A1	20-06-2002
			US 6348041 B1	19-02-2002
EP 0200919	A	12-11-1986	DE 3516052 A1	13-11-1986
			AT 44241 T	15-07-1989
			DE 3664107 D1	03-08-1989
			EP 0200919 A1	12-11-1986
WO 9607351	A	14-03-1996	AU 3212895 A	27-03-1996
			CA 2198909 A1	14-03-1996
			EP 0778746 A1	18-06-1997
			JP 10505269 T	26-05-1998
			WO 9607351 A1	14-03-1996
			US 2003040674 A1	27-02-2003
			US 2003018273 A1	23-01-2003
			US 5715827 A	10-02-1998
			US 6106476 A	22-08-2000

EPO FORM P0413

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82